

## Step One - Footplates

Before the child is in the stander, loosen the clamps (do not remove) on the footplates to adjust height (A). The knees should be slightly lower than the hips (B). Tighten clamps securely.



## Step Two - Seat Depth/Back Angle


Make adjustments before the child is in the stander. For easier adjustment, remove the Shadow Tray and bring seat up to a slight angle. If you have the Supine Option, make sure the supine locking handle is loose.

Loosen the knobs on the seat tube and the following arm (but do not unscrew completely).

**To adjust to a shorter seat depth setting,** adjust the following arm (back angle) first, by depressing the spring button and moving no more than two holes at a time. Then adjust the seat tube (seat depth) one hole at a time. Continue this sequence until you achieve the desired setting, and the colors on the seat tube and following arm match (C).

**Tip:**

- Position footplate height so the femur is resting on seat.



**To adjust to a longer seat depth setting,** adjust the seat tube (seat depth) first by depressing the spring button and moving only one hole at a time. Then adjust the following arm (back angle) no more than two holes at a time. Continue this sequence until you achieve the desired setting, and the colors on the seat tube and following arm match (C).

**Tips:**

- Remove Shadow Tray and bring seat up to a slight angle.
- Start with the smaller tube to adjust to a shorter setting.
- Start with the bigger tube to adjust to a longer setting.

For easier adjustment, use the seat bracket or the lift assist handle to lift slightly as the seat depth adjustment is made (D).

## Step Three - Kneepads

Position the user's hips as close as possible to stander's hip pivot (E). To determine correct positioning, fit two fingers between the front of the seat and the back of the knee (F). Adjust and secure the kneepads so the knees are centered in the pads.



**Tips:**

- Position child's hips in seat to match stander's hip pivot.
- You should be able to fit only 1-2 fingers behind the knee.

*For more detailed information refer to your owners manual.*

# EasyStand™ Bantam—Supine Option

## Supine Lever



The supine lever is located on the right side of the unit underneath the seat.




The lever should be flipped up to use the sit to stand function. The lever should be flipped down to use the supine function.

## Supine Locking Handle



The supine locking handle is located by the hip pivot on the left side of the unit.

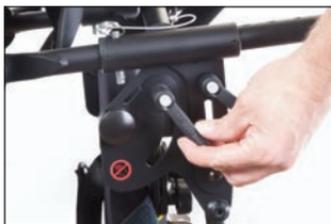

Handle must be loose (but not removed) for the sit-to-stand function, and tightened securely for the supine position.

## Foot Pedal



With the locking handle loose, recline the unit to the flat or desired position. Tighten the supine locking handle.



The stander is now ready for a flat-to-load transfer. Depress the foot pedal (or optional hydraulic pump) to position the stander at the desired standing angle.

*For more detailed information refer to your owners manual.*